


## E.STOP causes and methods of investigation


### ► Description

If the protection circuit is activated, here are possible causes and how to deal with them.

<b>Description</b>	When the protection circuit is activated, the buzzer sounds, the protection circuit activation indicator on the power amplifier system controller (SA-150) lights up, the protection circuit item is displayed on the 7-segment display, and the equipment automatically stops.
<b>Target series</b>	i-series/J-series /K-series

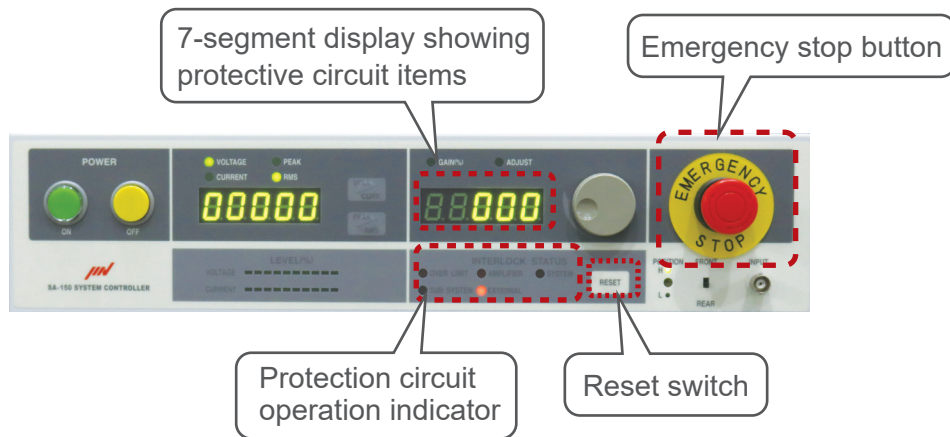


### • Error cause and remedy

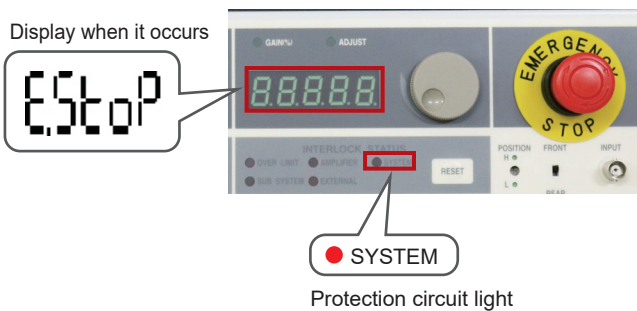

<b>Error</b>	Emergency stop
<b>Cause</b>	The emergency stop button is pressed.

If the emergency stop button is pressed, an E.STOP error will occur and the breaker will trip.

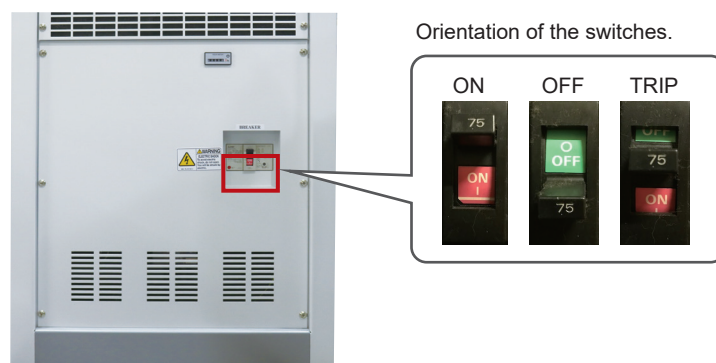




The emergency stop buttons are installed in the following locations.


1. Front of system controller (SA-150 and SA152)
  2. Near the vibration generator
  3. Interlocking device for vibration test system such as chamber
- \*2 and 3 are optional



Please turn all emergency stop buttons clockwise and then reset the main breaker.

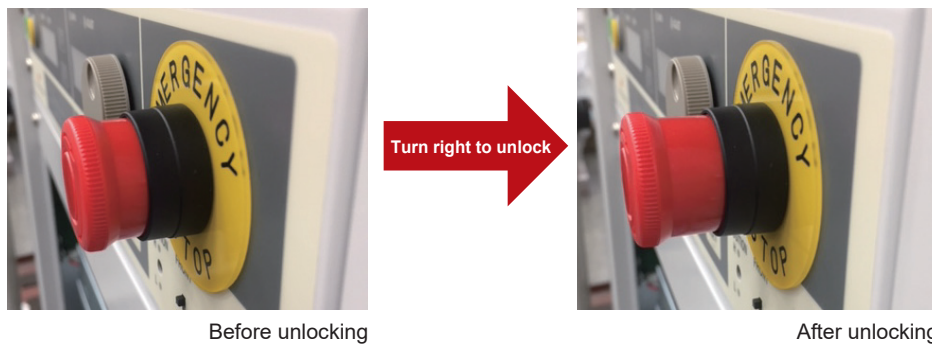

To reset the main breaker, turn it off first and then back on.

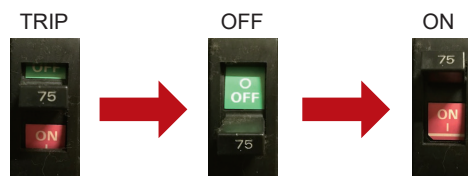

If the problem cannot be resolved, the vibration test system may be faulty.  
Please contact the IMV Service Centre.



Inquiries